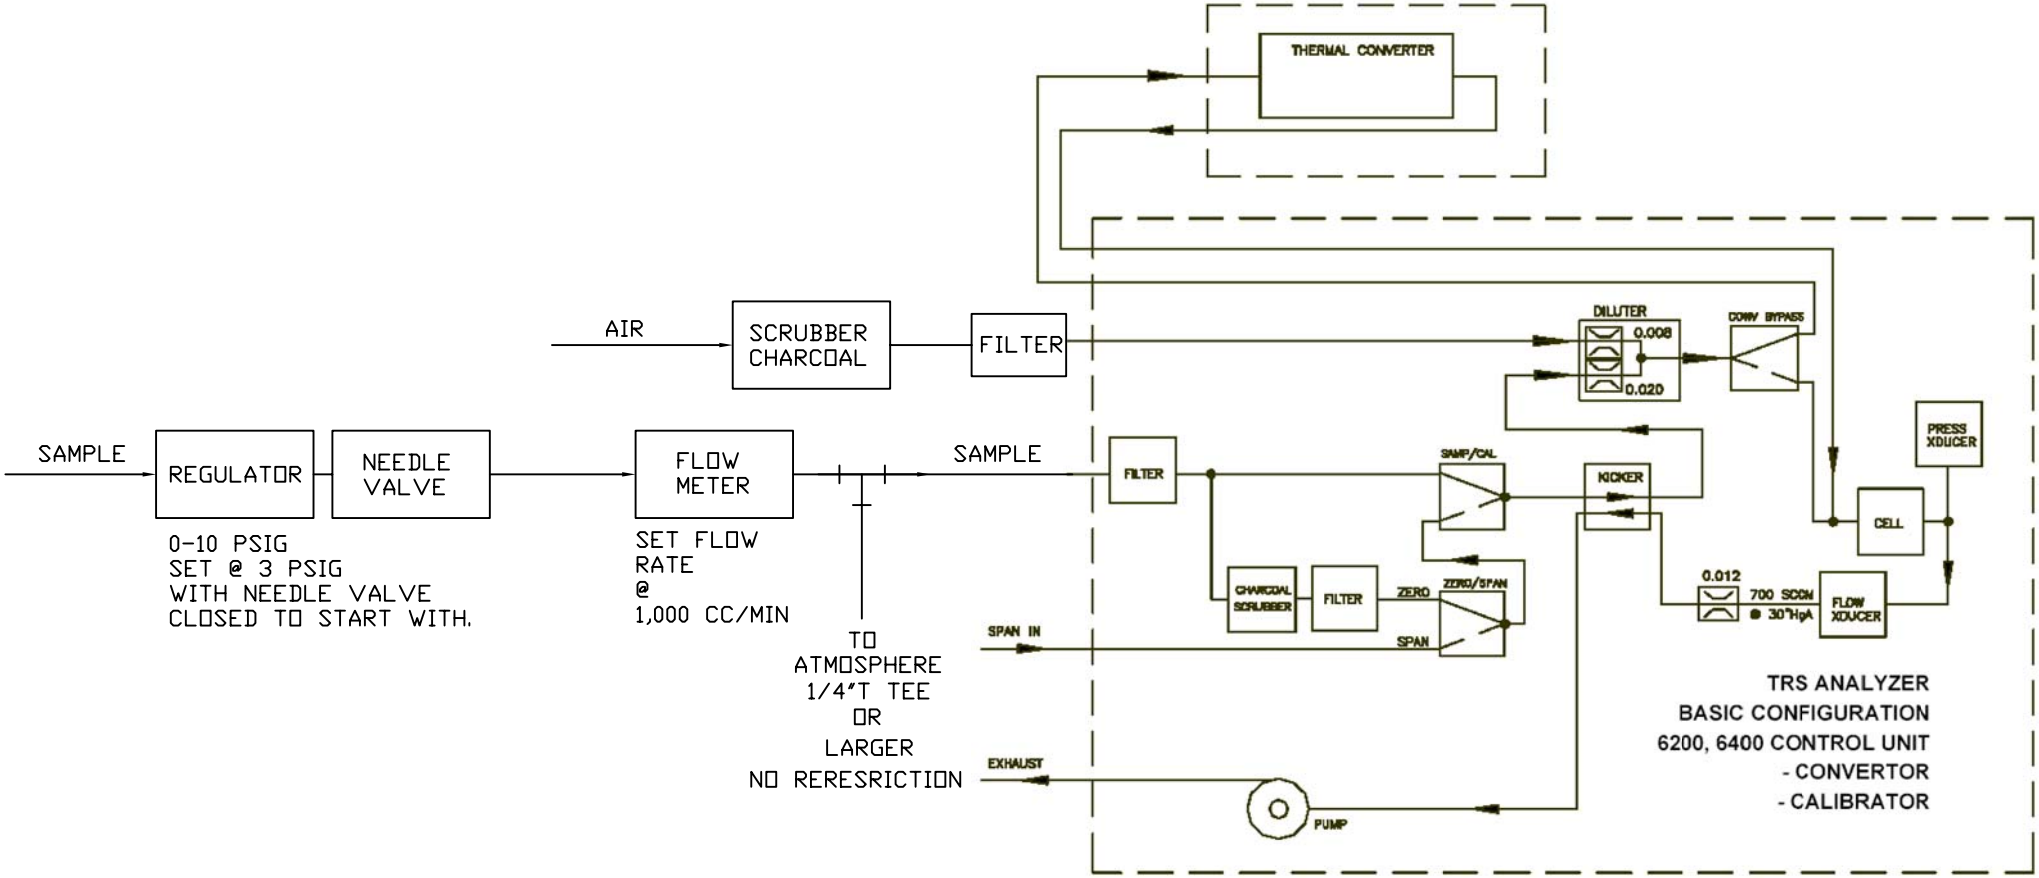
THERMAL CONVERTER
AIR
SCRUBBER CHARCOAL
FILTER
SAMPLE
REGULATOR
NEEDLE VALVE
0-10 PSIG
SET @ 3 PSIG
WITH NEEDLE VALVE
CLOSED TO START WITH.
FLOW METER
SET FLOW
RATE
@
1,000 CC/MIN
TO
ATMOSPHERE
1/4"T TEE
OR
LARGER
NO RERESRICTION
SAMPLE
FILTER
DILUTER
0.008
0.020
CONV BYPASS
SAMP/CAL
KICKER
PRESS XDUCER
CELL
CHARCOAL SCRUBBER
FILTER
ZERO
ZERO/SPAN
SPAN
SPAN IN
0.012
700 SCCM
@ 30"HgA
FLOW XDUCER
EXHAUST
PUMP
TRS ANALYZER
BASIC CONFIGURATION
6200, 6400 CONTROL UNIT
- CONVERTOR
- CALIBRATOR